



**2014-2015 Wet Weather WQO Ratios  
for S28 Dominguez Channel at Artesia Blvd.**

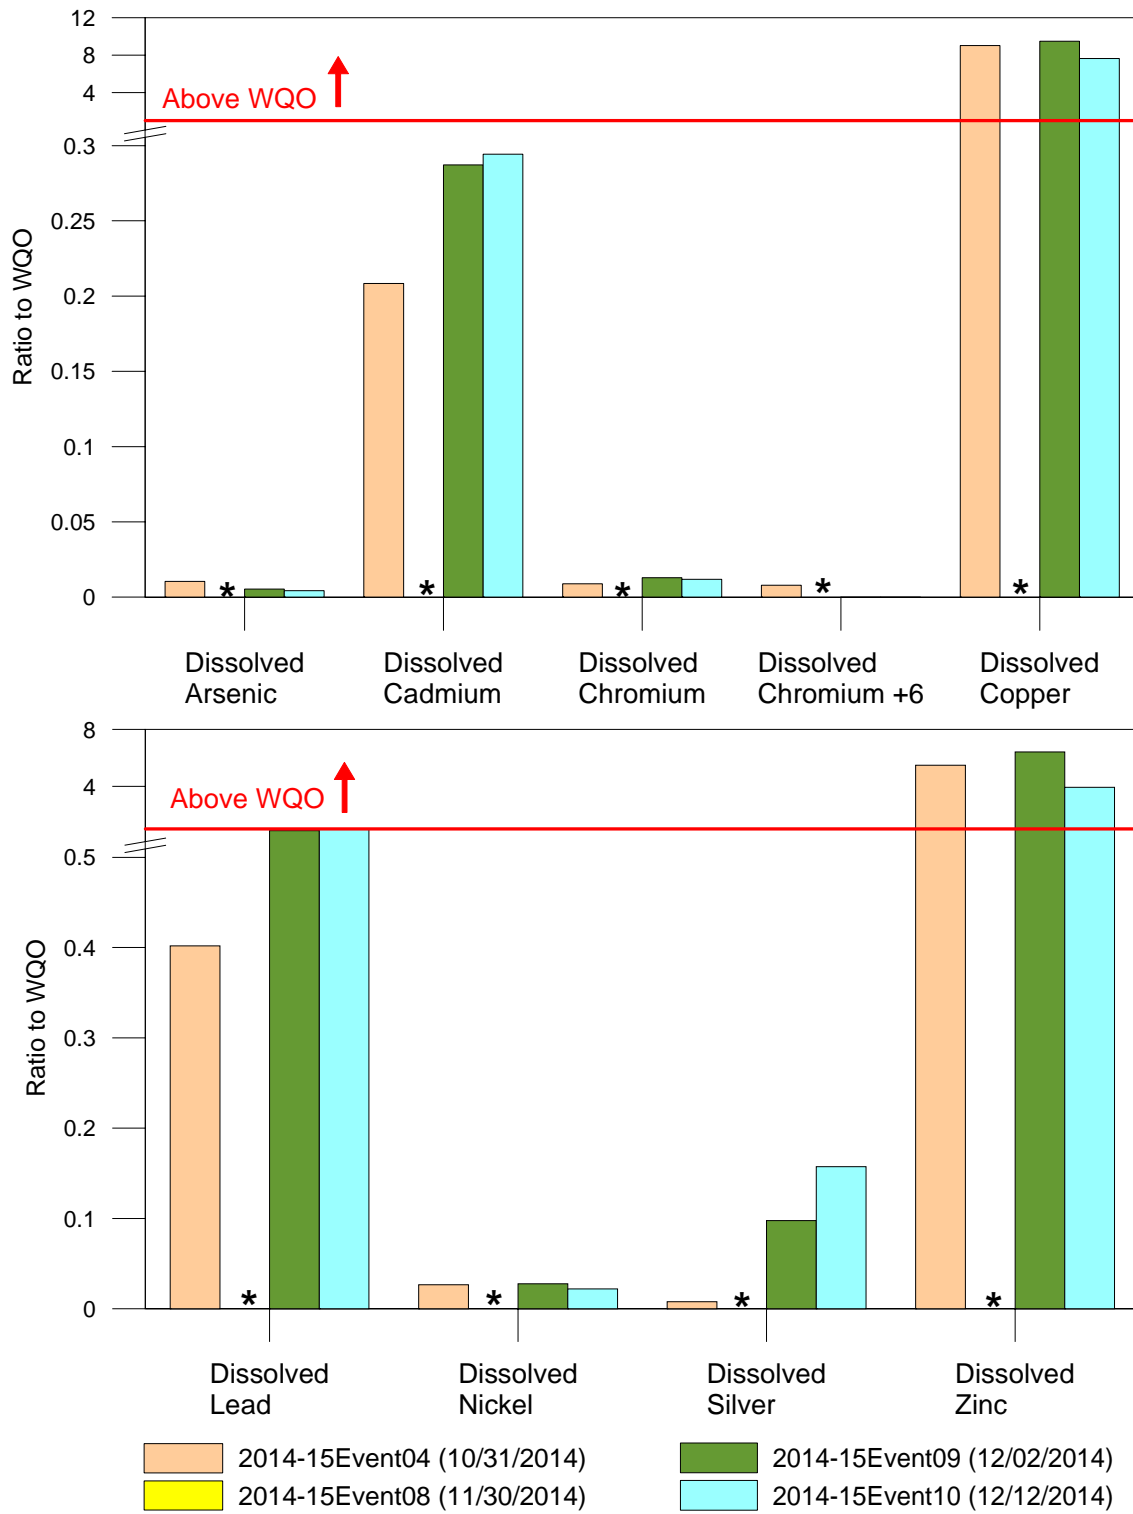

\*Samples were not collected for dissolved metals during Event 08.


Figure 4-3.6 S28 Dominguez Channel at Artesia Blvd Wet Weather Ratio Plots

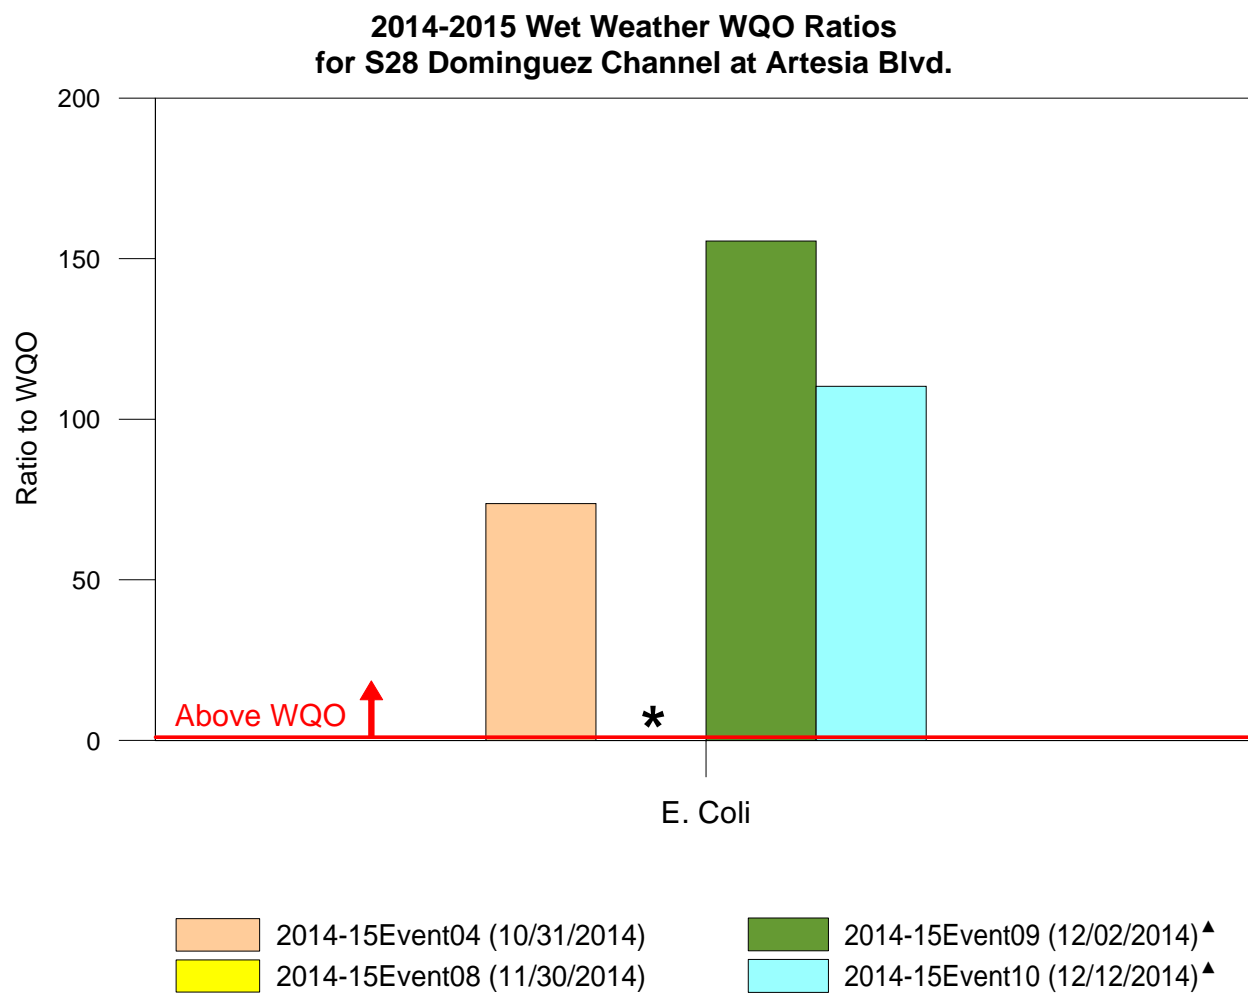

\*Samples were not collected for fecal coliforms during Event 08.

<sup>▲</sup>Not an exceedance of the E. coli water quality objective due to the High Flow Suspension of Recreational Uses (LARWQCB, 2003).

Figure 4-3.6 S28 Dominguez Channel at Artesia Blvd Wet Weather Ratio Plots

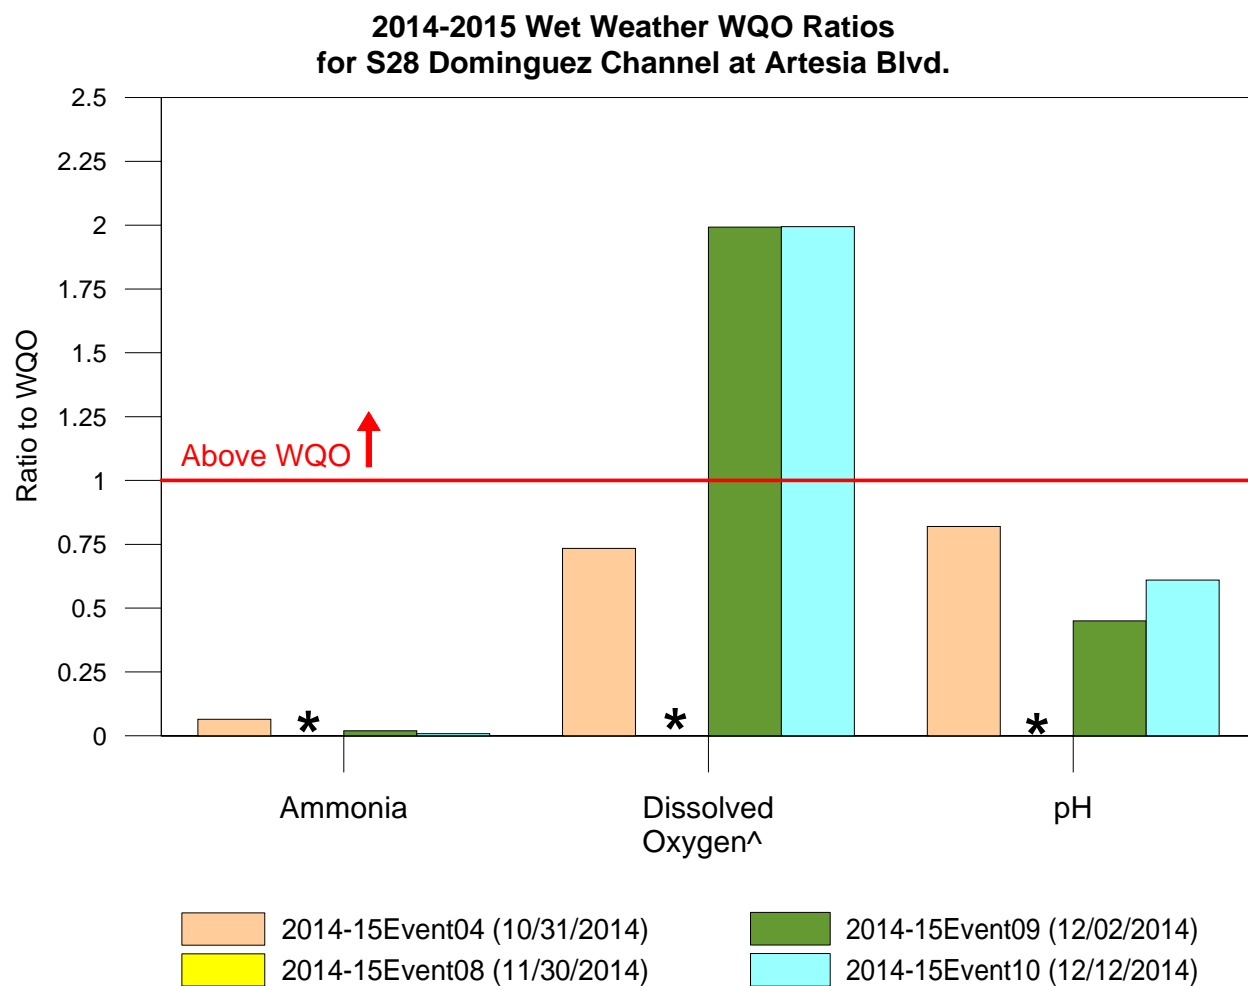

^Dissolved oxygen is an exceedance if ratio to WQO is below 1.

\*Samples were not collected for ammonia, dissolved oxygen or pH during Event 08.

Figure 4-3.6 S28 Dominguez Channel at Artesia Blvd Wet Weather Ratio Plots